

STORAGE AREA FOR:
AED SHOCK PADDLE ELECTRODES
AND OXIMETER ELECTRODE
(NONE SHOWN FOR CLARITY)

STORAGE AREA FOR:
AED SHOCK PADDLE ELECTRODES
AND OXIMETER ELECTRODE
(NONE SHOWN FOR CLARITY)

OXYGEN CYLINDER,
REGULATOR, GAUGE,
MASK AND HOSE
(MASK AND HOSE
NOT SHOWN
FOR CLARITY)

SPEAKER

REAR STORAGE AREA
FOR DC BATTERY,
(TERMINAL WIRES IN
BACK COMPARTMENT)

OXYGEN AND
PULSE DISPLAY
FOR OXIMETER


VOICE PROMPT
SELECTION/CONTROLS

OXIMETER CONTROLS

AED CONTROLS

LCD SCREEN

Fig. 2

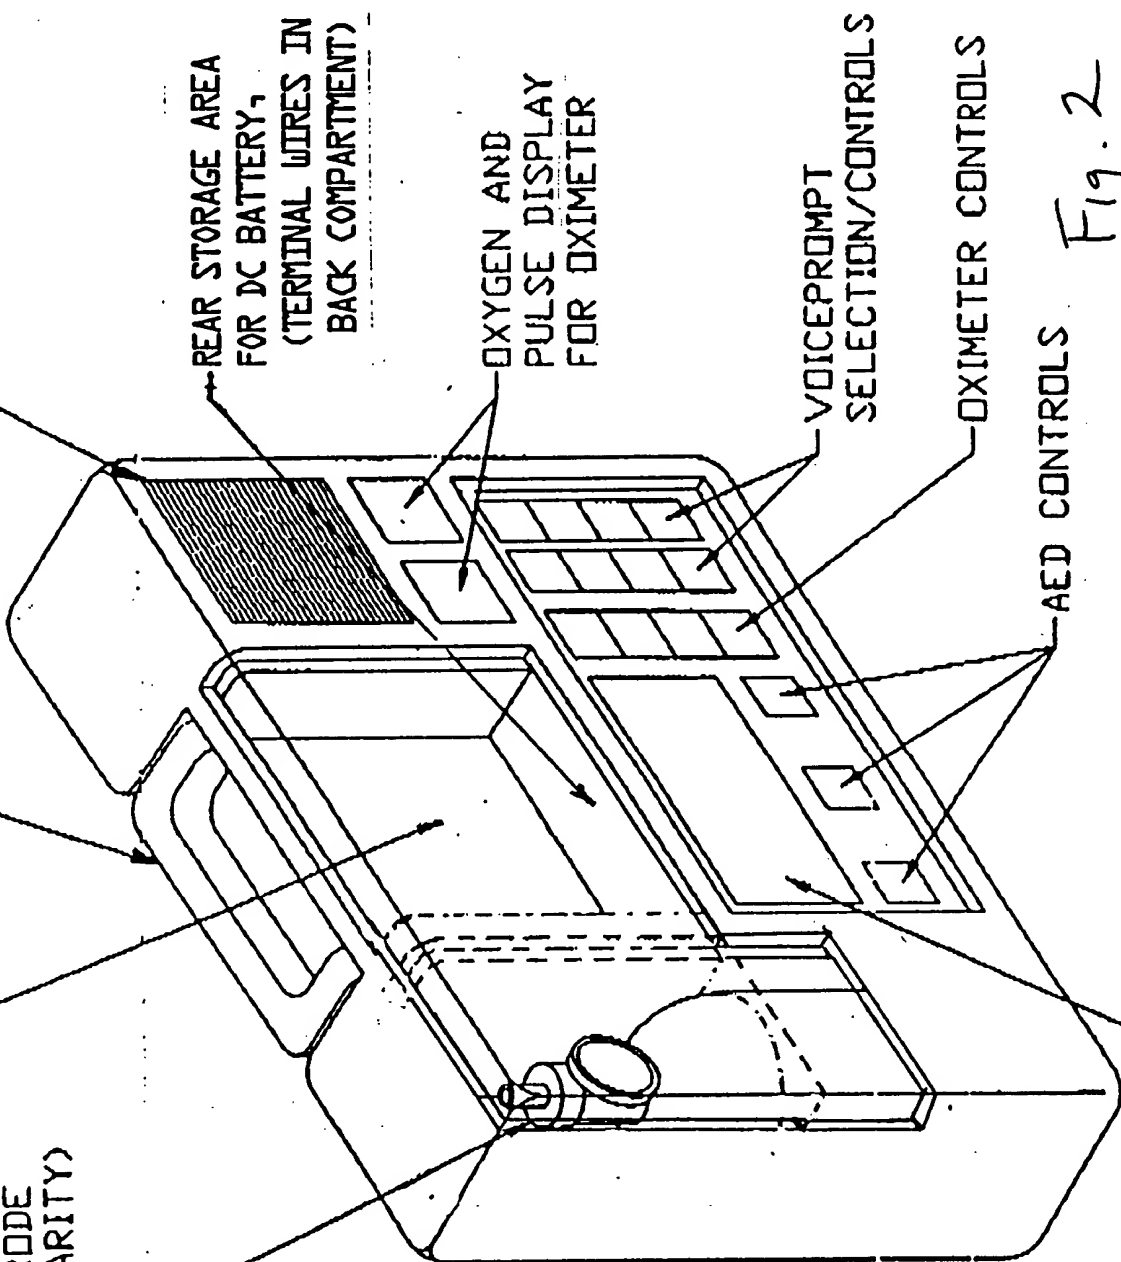

STORAGE AREA FOR:
AED SHOCK PADDE ELECTRODES
AND OXIMETER ELECTRODE
(NONE SHOWN FOR CLARITY)

OXYGEN CYLINDER,
REGULATOR, GAUGE,
MASK AND HOSE
MASK AND HOSE
NOT SHOWN
FOR CLARITY)

ALSO NOT SHOWN:
ELECTRO-MECHANICAL ON/OFF,
LITER FLOW-CONTROL,
PRESSURE CONTROL, AND
LITER FLOW/PRESSURE/TIME
SEQUENCING (VENTILATOR)

HANDLE

SPEAKER

REAR STORAGE AREA
FOR DC BATTERY,
(TERMINAL WIRES IN
BACK COMPARTMENT)

OXYGEN AND
PULSE DISPLAY
FOR OXIMETER

VOICEPROMPT
SELECTION/CONTROLS


OXIMETER CONTROLS

AED CONTROLS

LCD SCREEN

--- CARDIO-DIAGNOSIS & MONITORING
--- RESPIRATORY DIAGNOSIS & MONITORING
--- USER INSTRUCTIONS & PROMPTS

Fig. 3

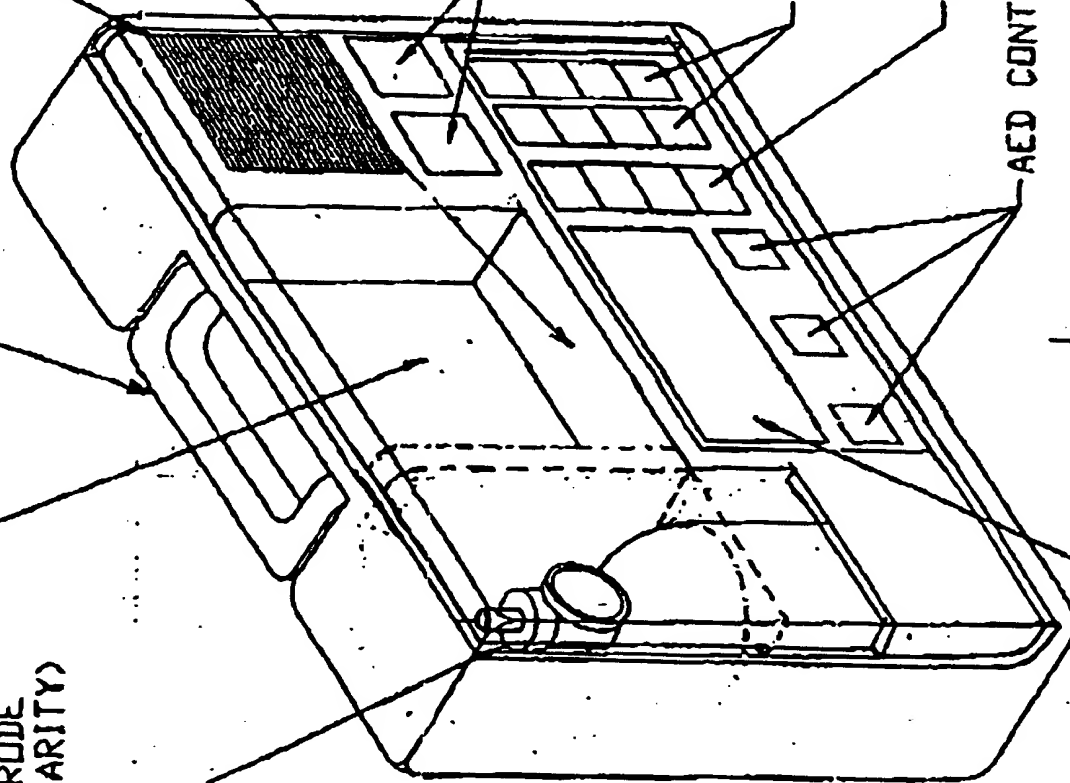

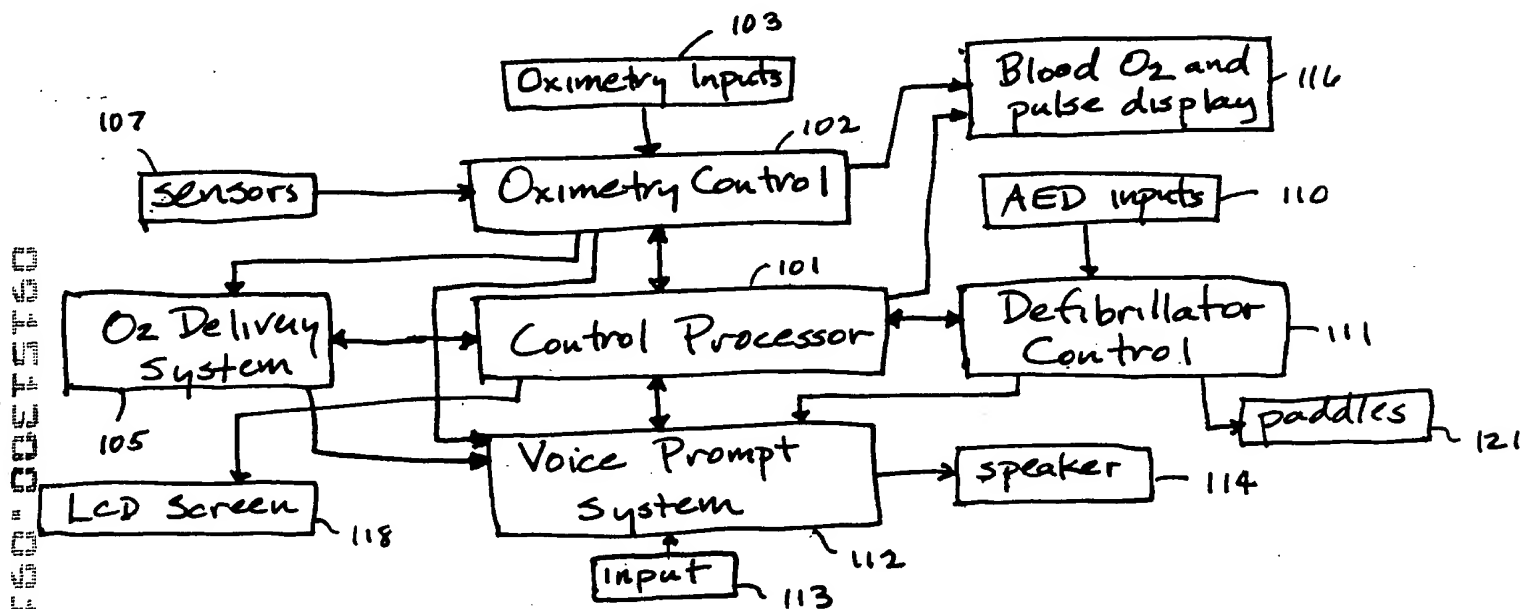


Fig. 4